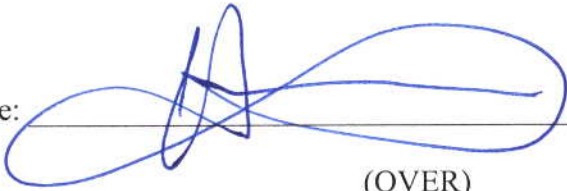



# VERIFICATION OF CALIBRATION REPORT

*Of DataMaster cdm Breath test Instrument*


*State of Alaska*

*Scientific Crime Detection Laboratory – Statewide Breath Alcohol Program*


DataMaster cdm S/N: <u>130193</u> ✓	
Supervisor/Operator Performing the Verification Procedure:	
Name: <u>JAMES C. GIPSON</u>	ID#: <u>4842</u> Date: <u>03 March 10</u> ✓
<b>A</b>	
Agency: <u>Palmer Police Department</u>	Phone #: <u>(907) 745-4811</u>
Instrument Location: <u>Palmer Police Department</u> ✓	
<b>B</b>	
Alco S/N: <u>77621</u> ✓	Target Value: <u>.079</u> ✓ High Pressure: <u>925</u>
Alco Test Value Average:	<u>.079</u> ✓ <u>.078</u> ✓
	1 <sup>st</sup> Alco 2 <sup>nd</sup> Alco
Signature: 	
(OVER)	

I, Nita J. Bolz, after being first duly sworn, depose and state as follows. (Do Not write in the area below)

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

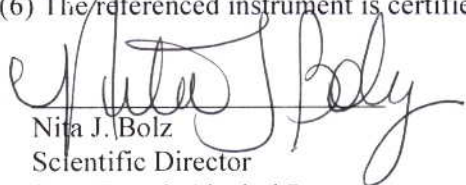  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 21<sup>st</sup> day of March, 2010.

  
(Notary Seal Stamp)

Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office

